


PS



INGUINAL HERNIA

CŒLIOSCOPY

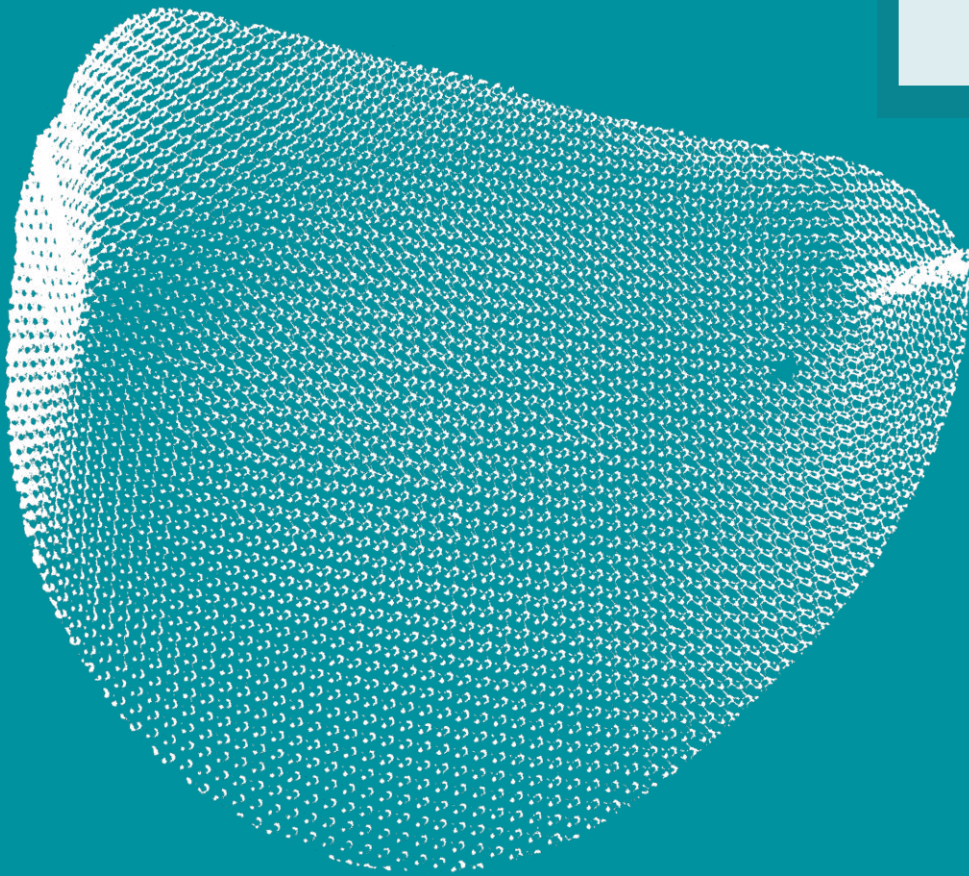

*Tridimensional implant
for TEP or TAPP surgeries.*

90G / M²
POROSITY > 77%



90G / M²
POROSITY > 77%



	cm	STANDARD POLYPROPYLENE	BULMESH POLYPROPYLENE
	11x15	413 150	
	10x16	413 160	601 160 ^R 601 161 ^L
	11x16.5	413 165	

R - right / L - left